


Lab Notebook Entry from LeCroy DSO
DSO S/N: LCRY0719N52716
User: LeCroyUser
Time: 8/9/2019 2:04:54 PM

MyLabNotebook--00026



LabNotebook

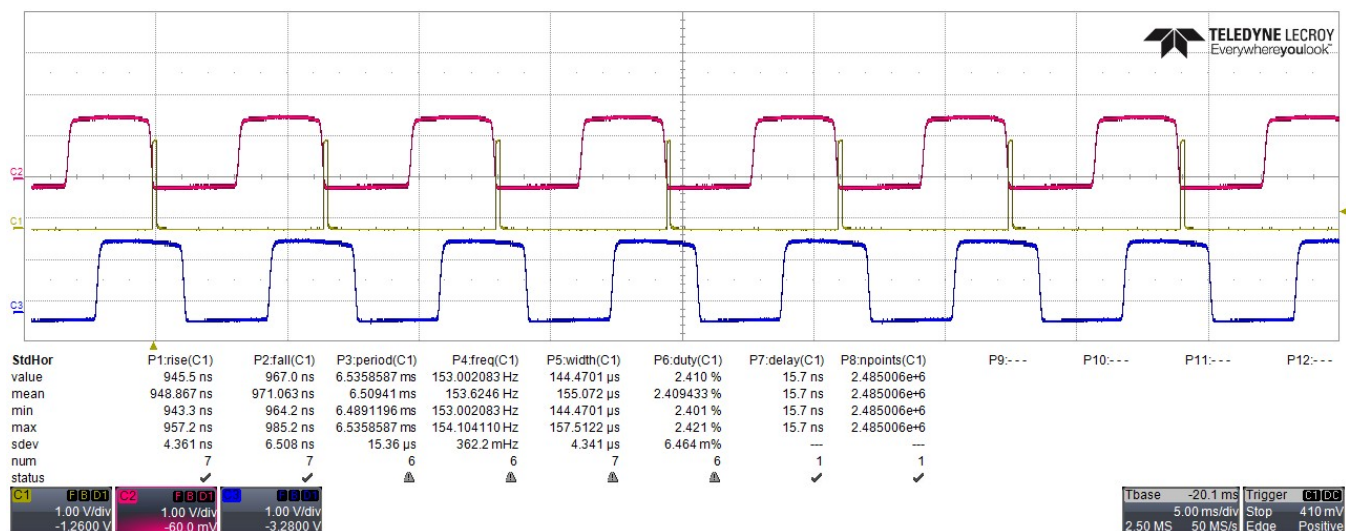

Channel Status

	C1	C2	C3
V / Div	1.00 V	1.00 V	1.00 V
Offset	-1.2600 V	-60.0 mV	-3.2800 V
Coupling	DC1M Ω	DC1M Ω	DC1M Ω
BW-Limit	200MHZ	200MHZ	20MHZ
Probe	10	10	10
Sweeps	1 #	1 #	1 #

Acquisition Status

Horizontal	Time / Div	5.00 ms	Sampling Rate	50.000000 MS/s
	Time / Pt	20.000000 ns	Sampling Mode	RealTime
	Pts / Div	250.0000 kS	Trigger Delay	-20.1 ms
Trigger	Mode	Stop	Slope	Positive
	Type	Edge	Level	410 mV
	Source	C1	Coupling	DC